



DYNA

ISSN: 0012-7353

Universidad Nacional de Colombia

Duarte Guedes Cabral de Almeida, Ceres; Oliveira Silva, Denize Maria; Gomes de Almeida, Brivaldo; de França e Silva, Ênio Farias; Neves Barbosa, Rebeca; Santos Júnior, José Amilton

FDR ECH2O sensor performance in Spodosols

DYNA, vol. 85, no. 207, 2018, October-December, pp. 60-64

Universidad Nacional de Colombia

DOI: <https://doi.org/10.15446/dyna.v85n207.71897>

Available in: <https://www.redalyc.org/articulo.oa?id=49658894008>

- How to cite
- Complete issue
- More information about this article
- Journal's webpage in redalyc.org

UNEN 

Scientific Information System Redalyc

Network of Scientific Journals from Latin America and the Caribbean, Spain and Portugal

Project academic non-profit, developed under the open access initiative

## FDR ECH<sub>2</sub>O sensor performance in Spodosols

Ceres Duarte Guedes Cabral de Almeida <sup>a</sup>, Denize Maria Oliveira Silva <sup>b</sup>, Brivaldo Gomes de Almeida <sup>c</sup>,  
Ênio Farias de França e Silva <sup>b</sup>, Rebeca Neves Barbosa <sup>c</sup> & José Amilton Santos Júnior <sup>b</sup>

<sup>a</sup> Colégio Agrícola Dom Agostinho Ikas, Universidade Federal Rural de Pernambuco, São Lourenço da Mata, Brasil. [ceres.cabral@ufrpe.br](mailto:ceres.cabral@ufrpe.br)

<sup>b</sup> Departamento de Engenharia Agrícola, Universidade Federal Rural de Pernambuco, Recife, Brasil. [denize.etr@gmail.com](mailto:denize.etr@gmail.com), [enio.silva@deagri.ufrpe.br](mailto:enio.silva@deagri.ufrpe.br), [joseamilton@ufrpe.br](mailto:joseamilton@ufrpe.br)

<sup>c</sup> Departamento de Agronomia, Universidade Federal Rural de Pernambuco, Recife, Brasil. [brivaldo.almeida@ufrpe.br](mailto:brivaldo.almeida@ufrpe.br), [rebecanb01@gmail.com](mailto:rebecanb01@gmail.com)

Received: April 25<sup>th</sup> de 2018. Received in revised form: August 31<sup>th</sup> 2018. Accepted: September 24<sup>th</sup>, 2018

### Abstract

Frequency domain reflectometry (FDR) is widely used to measure soil water content. However, the effects of soil composition on FDR calibration have to be quantified to reduce the need for further calibration. Our objectives were to: (1) evaluate the accuracy of EC-5 for measuring water content in sandy soils, and (2) develop a soil-specific sensor calibration curve. Disturbed and undisturbed soil samples were collected in one Spodosol profile (07° 37' 30" S, 34° 57' 30" W) representative of the region where sugarcane is grown in northeastern Brazil. Regression analysis showed good accuracy and low error (RMSE = 0.01 m<sup>3</sup> m<sup>-3</sup>), while without specific calibration the error was higher (RMSE = 0.06 m<sup>3</sup> m<sup>-3</sup>). The EC-5 sensor should be subjected to field-specific calibration in sandy soils due to the low field capacity and water content during the growing season.

**Keywords:** EC-5; sandy soil; volumetric water content; probe; capacitance.

## Desempeño de un sensor FDR ECH<sub>2</sub>O en Espodosuelos

### Resumen

La Reflectometría en el Dominio de Frecuencia (FDR) es ampliamente utilizada para medir el contenido de agua en el suelo. Sin embargo los efectos de la composición del suelo en la calibración de FDR deben de cuantificarse para reducir la necesidad de una calibración adicional. Nuestros objetivos fueron: (1) evaluar la precisión del sensor EC-5 para medir el contenido de agua en suelos arenosos y (2) desarrollar la curva de calibración del sensor específica del suelo. Muestras de suelo disturbadas y no disturbadas fueron recogidas en un perfil de Spodosol (07° 37' 30" S, 34° 57' 30" W) representativo de una región productora de caña de azúcar, en el Noreste de Brasil. Los resultados del análisis de regresión mostraron una buena precisión y bajo error (RMSE = 0.01 m<sup>3</sup> m<sup>-3</sup>), mientras que sin calibración específica el error fue mayor (RMSE = 0.06 m<sup>3</sup> m<sup>-3</sup>). El sensor EC-5 debe de someterse a calibración específica en el campo en suelos arenosos debido a la baja capacidad de campo y contenido de agua en el periodo de crecimiento de la planta.

**Palabras clave:** EC-5; suelo arenoso; contenido volumétrico de agua; sonda; capacitancia.

### 1. Introduction

Irrigation is a technique that allows farmers to provide food for large populations, but it also consumes large quantities of water and energy. The amount of water lost through this process is affected by irrigation system design and irrigation management. However, optimizing the use of water is one way to reduce irrigation costs. Irrigation scheduling, which is the process of determining when to irrigate and how much water to apply, if done prudently, minimizes runoff and percolation losses, which in turn usually maximizes irrigation efficiency by reducing energy

and water use. Soil moisture monitoring is a necessary safeguard to assure that soil moisture levels are adequate [1,2].

Monitoring soil volumetric water content (VWC) and its availability are needed to support plant growth and characterize soil water evaporation. There are several methods available that can estimate in situ soil water content. These methods include time domain reflectometry (TDR), Reflectometry Frequency Domain (FDR), neutron probe, and tensiometers [3-6]. The gravimetric method, which is the oldest method, is disadvantaged by the time and effort required to obtain data, and it does not allow for real-time

**How to cite:** de Almeida, C.D.G.C., Silva, D.M.O., de Almeida, B.G., Silva, E.F.deF., Barbosa., R.N. and Santos., J.A.Jr., FDR ECH<sub>2</sub>O sensor performance in Spodosols. DYNÁ, 85(207), pp. 60-64, Octubre - Diciembre, 2018.

measurement of water content. However, it continues being widely used for obtaining soil moisture data; it is required for calibrating the equipment used in the other methods because it is the only direct way of measuring soil moisture, and is also the most accurate method [7]. However, non-destructive monitoring methods have become increasingly required for environmental evaluation, precision agriculture, and natural resources management [8]. For this reason, several studies have been performed on instruments for indirect measurement, but few have been conducted for specific soils in Brazil.

ECH<sub>2</sub>O probes are capacitance sensors that measure the volumetric water content of the soil by measuring the dielectric constant of the soil, which is a direct function of water content. However, soils do not have identical electrical properties. Due to variations in soil bulk density, mineralogy, texture, and salinity, specific mineral calibration for current ECH<sub>2</sub>O sensors is necessary [9].

Temperature effects on dielectric permittivity measurements are significant under field conditions and occur especially in the upper soil horizon where the soil temperature is influenced by diurnal and seasonal temperature fluctuations [10].

The EC-5 is part of the ECH<sub>2</sub>O group of Decagon Devices and was developed to be much less sensitive to variation in texture and electrical conductivity because it works with a frequency of 70 MHz. Therefore, its general calibration equation should apply for all mineral soils up to 8 dS m<sup>-1</sup> saturation extract [11].

The need for a specific calibration of the sensor for each site is one the most important reasons why the use of this equipment is not more widespread. In addition to the time and effort required, they can be expensive for the farmers. One option is that laboratory calibrations be conducted on typical agricultural soils. This will allow farmers to use more accurate calibration equations than those specified by the manufacturer, tailored to the general type of soil that they are farming. And it will restrict the need for site-specific calibration to only extreme instances of soil abnormality [12]. Sandy soils are extensively distributed in Coastal Tablelands ecosystems in Northeast Brazil. Despite the difficulties involved in utilizing sandy soils, this region is among the top-ranked regions for agricultural production in Brazil.

The ECH<sub>2</sub>O EC-5 sensor is a promising soil moisture sensor for sandy soils. Our objectives were to: (1) evaluate the accuracy of EC-5 for measuring soil water content in sandy soils, and (2) develop soil-specific sensor calibration curve.

## 2. Materials and methods

This study was carried out in a greenhouse at the Federal Rural University of Pernambuco, in Northeast of Brazil (08° 01' 07" S, 34° 56' 53" W, and mean altitude of 6,50 m). According to the Köppen classification, the climate of this region is As, with annual average precipitation of 1,501 mm, average temperature of 26°C, and relative humidity of 76%.

Disturbed and undisturbed soil samples were collected at Goiana City (07° 37' 30" S, 34° 57' 30" W), which is representative of sugarcane grown in Coastal Tablelands

ecosystems, in the Experimental Station of Itapirema belonging to Agronomic Institute of Pernambuco (IPA). This soil was classified as Spodosol Humiluvic orthic [13], which is very sandy (sand = 859 g kg<sup>-1</sup>; silt = 25 g kg<sup>-1</sup>; clay = 116 g kg<sup>-1</sup>). Both disturbed and undisturbed soil samples were taken from the upper 40 cm. Undisturbed samples were collected in stainless steel cores (5 x 5 cm, inside diameter and height) inserted into the field by an Uhland-modified sampler. Disturbed soil samples were air-dried and ground to pass through a 4.75 mm sieve, then packed in six 5.00 L volume plastic containers. A gravel layer and drainage fabric were put in the bottom of each container, leaving 4.66 L volume available. The samples were saturated by capillarity and then put on a table for water drainage until they reached a field capacity, when they were weighed. One EC-5 sensor (Decagon Devices, Inc.) was placed vertically into each container together with the soil material. A specific amount of soil was prepared for each container to obtain the same bulk density as was measured in the undisturbed soil samples (1.56 g cm<sup>-3</sup>). Each probe was connected to a EM50 (Decagon Devices, Inc.) to record data daily at 7:00am, 12:00pm, and 4:00pm over 37 days, up to when the difference between successive weight measurements remained constant. As recommended by manufacture, ECH<sub>2</sub>O Utility software was used to connect and configure EM50. This software allows the user to select the output unit of the sensor measurements (mV, m<sup>3</sup> m<sup>-3</sup>, cm<sup>3</sup> cm<sup>-3</sup>, %, inches per foot). In this work, we chose m<sup>3</sup> m<sup>-3</sup>, which is volumetric water content measured by the sensor and based on the manufacturer's calibration equation.

In addition to volumetric water content (not discussed in this study), the 5TE sensor (Decagon Devices, Pullman, WA) provides data on soil temperature and electrical conductivity. Three sensors were inserted vertically into three containers to measure temperature and electrical conductivity hourly. These sensors were connected to an EM50 as well.

Gravimetric method, which is the only direct reference method for the calibration process of this sensor, was used to determine volumetric soil water content by eq. (1):

$$\theta = U \times BD \quad (1)$$

Where:  $\theta$  is volumetric soil water content, expressed in m<sup>3</sup> m<sup>-3</sup>;  $U$  is gravimetric soil water content, expressed in kg kg<sup>-1</sup>; and  $BD$  is bulk density g cm<sup>-3</sup>.

Linear regression fits were then used to relate measurements of obtained volumetric soil water,  $Y$  (m<sup>3</sup> m<sup>-3</sup>), and volumetric soil water estimated by sensors,  $X$  (m<sup>3</sup> m<sup>-3</sup>), based on manufacture calibration. Data were analyzed and interpreted by analysis of variance and regression analysis. A 0.05 significance level was used in all statistical tests.

Four statistical measures were computed to evaluate and compare each equation-predicted value (sensor) with the observed value derived from gravimetric moisture taken from the laboratory soils. These included the coefficient of determination ( $R^2$ ), mean bias error (MBE), root mean square error (RMSE), and the index of agreement ( $d$ ) as defined by [14] and shown in eq. (2).

$$d = 1 - \left[ \frac{\sum (P_i - O_i)^2}{\sum (|P_i - O| + |O_i - O|)^2} \right] \quad (2)$$

Where:  $P_i$  is the estimated value,  $O_i$  is the determined value, and  $O$  is the mean determined value.

### 3. Results and discussion

According to the F-test in analysis of variance (ANOVA), measured VWC and EC-5 estimated VWC, as calibrated by the manufacturer, were significant as shown Table 1.

However, Table 2 shows there were no significant differences by F-test in ANOVA between measured VWC and EC-5 estimated VWC, calibrated with the laboratory equation.

The loss of soil water by natural drying is shown in Fig. 1. The figure shows soil moisture average in the six containers, according to readings of the six EC-5 sensors and also the gravimetric data, which were converted to volumetric water contents using the soil bulk density.

Table 1.

Variance analysis of measured VWC and EC-5 estimated VWC, as calibrated by manufacturer.

Source of variation	Degree of freedom	Mean Square	F	P value	F critical value
Between	1	0.168	15.129	0.0001	3.882
Within	230	2.558			

Source: The authors.

Table 2.

Variance analysis of measured VWC and EC-5 estimated VWC, calibrated by laboratory equation.

Source of variation	Degrees of freedom	Mean Square	F	P value	F critical value
Between	1	$1.232 \cdot 10^{-07}$	$1.164 \cdot 10^{-5}$	0.997	3.882
Within	230	2.436			

Source: The authors

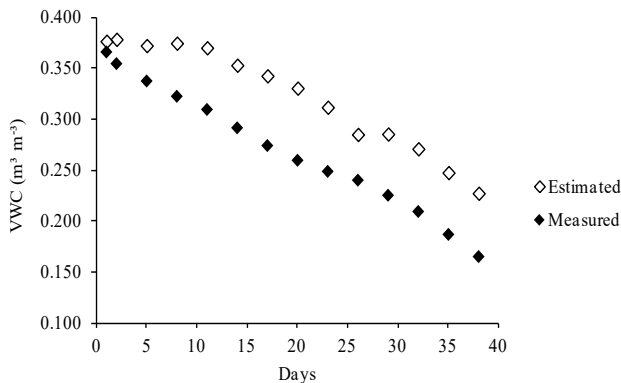


Figure 1. Depletion of soil moisture (drying curve) estimated by EC-5 sensor (according to manufacturer's calibration) and measured gravimetrically (converted to volumetric soil water content) during the monitored period. Source: The authors.

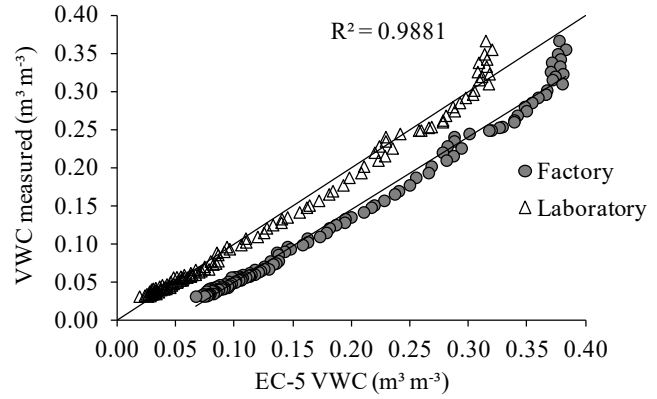


Figure 2. Comparison between factory-calibrated and laboratory-calibrated  $\theta$  estimated by the EC-5 sensor.

Source: The authors.

In the evaluated moisture range, the moisture values obtained using the manufacturer's calibration were overestimated, relative to those obtained by weighing. The mean estimated value ranged from an initial volumetric moisture  $0.377 \text{ m}^3 \text{ m}^{-3}$  to a maximum of  $0.067 \text{ m}^3 \text{ m}^{-3}$ . The mean determined value, however, ranged from  $0.367 \text{ m}^3 \text{ m}^{-3}$  to  $0.0314 \text{ m}^3 \text{ m}^{-3}$ .

A linear calibration equation, here referred to as the 'laboratory calibration' of  $\theta$ , was developed for EC-5 sensor by plotting the probes readings versus the  $\theta$  derived from the gravimetric method. The equation was developed using the Microsoft Excel® Regression which is showed in eq. (3) below.

$$\theta = 0.953X - 0.0451 \quad (3)$$

Where:  $\theta$  is expressed in  $\text{m}^3 \text{ m}^{-3}$ ; 0.953 (slope) and -0.0451 (intercept) are fitted coefficients; and  $X$  is the sensor-based factory calibration of  $\theta$  ( $\text{m}^3 \text{ m}^{-3}$ ).

Measured data and the resulting laboratory calibration equation are shown in Fig. 2.

The laboratory calibration equation reflects that the variables explained 98.81% of the variability in the  $a$  and  $b$  parameters and very good correlation was obtained. The laboratory calibration of  $\theta$  for the EC-5 sensor closely matched the one-to-one line. This suggested an accurate calibration for the sandy soil, with some scatter at the higher water content range ( $0.310$ – $0.366 \text{ m}^3 \text{ m}^{-3}$ ). The difference between soil water content predicted by specific calibration and gravimetrically derived volumetric soil water content ranged from  $0.018$  to  $-0.052 \text{ m}^3 \text{ m}^{-3}$ , where the positive values demonstrate overestimation of the moisture by the adjustment equation and the negative ones show the inverse. These results agree with [15], which showed a linear soil-specific calibration for sandy clay loam soil using a 5TE sensor.

The factory calibration applied to the data collected from the EC-5 sensors overestimated  $\theta$  by  $0.090 \text{ m}^3 \text{ m}^{-3}$  (MBE), and resulted in an RMSE of  $0.06 \text{ m}^3 \text{ m}^{-3}$ . However, laboratory calibration improved accuracy at EC-5 in this soil, with a lower RMSE ( $0.01 \text{ m}^3 \text{ m}^{-3}$ ) and a higher index of agreement ( $d=0.9770$ ), which reflects the high accuracy with which the determined volumetric moisture is estimated by the specific

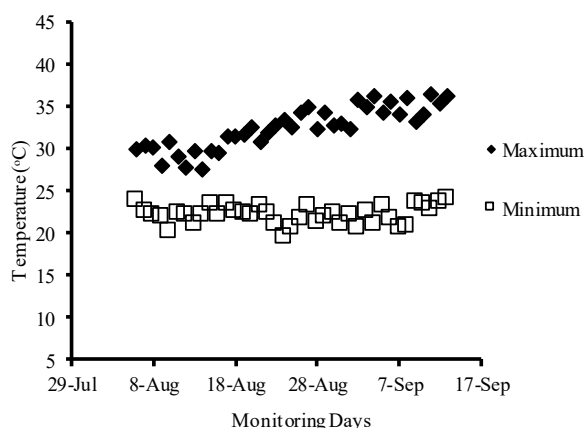


Figure 3. Soil temperature maximum and minimum estimated by the 5TE sensor.

Source: The authors.

calibration. This is in agreement with findings made by [15] that the factory calibration for the 5TE also overestimate  $\theta$  mainly at the large water contents and field based calibration equation is satisfactory to achieve the required accuracy of this sensor.

Soil texture has important role in temperature and water content variation. In sandy soils surface is not recommended the use of moisture soil sensors, due to the largest fluctuations of parameters. It is also suggested that users of the probes perform their own calibration for their particular application [3].

It is evident that sensor requires unique calibrations for the soil and conditions in which it will operate. Then, it is recommended that laboratory calibration be developed, over factory calibration, since soil specific data are more representative.

The maximum soil temperature ranged from 27.6 to 36.4°C, while the minimum ranged from 19.6 to 24.2°C. Fluctuations in the maximum temperatures were higher than in the minimum, which were more homogeneous (Fig. 3).

Saline soils have an electrical conductivity of saturated extract (EC<sub>se</sub>)  $\geq 4.0$  dS m<sup>-1</sup> [16]. In this study, Spodosol mean electrical conductivity estimated by the 5TE sensor was 0.030 dS m<sup>-1</sup>, thus it is not considered saline soil and the probe can be used.

#### 4. Conclusions

This research evaluated the performance of EC-5 soil water content sensor since saturation to drier range, under laboratory conditions for Spodosol which is representative of sugarcane grown in Coastal Tablelands ecosystems.

The EC-5 sensor for measuring soil water content tested in this study appeared to be very sensitive and suitable for continuous measurements soil water content.

The study of the EC-5 has shown that factory calibration of the probe overestimated the volumetric water content and therefore should be substituted by a laboratory calibration.

When fitting the EC-5 sensor readings versus the  $\theta$  derived from the gravimetric method obtained very good correlation with linear equation ( $R^2 = 0.9881$ ).

Acceptable sensor error for these tests was set to less than 0.011 m<sup>3</sup>m<sup>-3</sup> for the RMSE.

#### References

- [1] Evans, R., Sneed, R.E. and Cassel, D.K., Irrigation scheduling to improve water and energy use efficiencies. North Carolina Cooperative Extension Service [Online], AG 452-4, 1996. [date of reference: April 4<sup>th</sup> of 2018]. Available at: <https://content.ces.ncsu.edu/irrigation-scheduling-to-improve-water-and-energy-use-efficiency>
- [2] Evans, R., Sneed, R.E. and Hunt, J.H., Irrigation management strategies to improve water and energy-use efficiencies. North Carolina Cooperative Extension Service [Online], AG 452-5, 1996. [date of reference: March 6<sup>th</sup> of 2018]. Available at: <https://content.ces.ncsu.edu/irrigation-management-strategies-to-improve-water-and-energy-use-efficiencies>
- [3] McMichael, B. and Lascano, R.J., Laboratory evaluation of a commercial dielectric soil water sensor. *Vadose Zone Journal*, 2(4), pp. 650-654, 2003. DOI: 10.2136/vzj2003.6500
- [4] Kinzli, K., Manana, N. and Oad, R., Comparison of laboratory and field calibration of a soil-moisture capacitance probe for various soils. *Journal of Irrigation and Drainage Engineering*, 138(4), pp. 310-321, 2012. DOI: 10.1061/(ASCE)IR.1943-4774.0000418.
- [5] Mittelbach, H., Lehner, I. and Seneviratne, S.I., Comparison of four soil moisture sensor types under field conditions in Switzerland. *Journal of Hydrology*, 430, pp. 39-49, 2012. DOI: 10.1016/j.jhydrol.2012.01.041.
- [6] Kodešová, R., Kodeš, V. and Mraz, A., Comparison of two sensors ECH<sub>2</sub>O EC-5 and SM200 for measuring soil water content. *Soil and Water Research*, 6(2), pp. 102-110, 2011. DOI: 10.17221/6/2011-SWR
- [7] Johnson, A.I., Methods of measuring soil moisture in the field. Washington, United States Government Printing Office, 1962, 29 P.
- [8] Saito, T., Fujimaki, H. and Inoue, M., Calibration and simultaneous monitoring of soil water content and salinity with capacitance and four-electrode probes. *American Journal of Environmental Sciences*, 4(6), pp. 683-692, 2008. DOI: 10.3844/ajessp.2008.683.692
- [9] Cobos, D.R. and Chambers, C., Calibrating ECH<sub>2</sub>O soil moisture sensors application note. Pullman, Washington, Decagon Devices Inc., 2010, 7 P.
- [10] Jones, S.B., Blonquist, J.M., Robinson, D.A., Rasmussen, V.P. and Or, D., Standardizing characterization of electromagnetic water content sensors. *Vadose Zone Journal*, 4(4), pp. 1048-1058, 2005. DOI: 10.2136/vzj2004.0140
- [11] Decagon Devices Inc., EC-5 soil moisture sensor: Operator's Manual. Pullman, Washington, Decagon Devices Inc., 2016, 22 P.
- [12] Spelman, D., Kinzli, K. and Kunberger, T., Calibration of the 10HS soil moisture sensor for Southwest Florida agricultural soils. *Journal of Irrigation and Drainage Engineering*, 139(12), pp. 965-971, 2013. DOI: 10.1061/(ASCE)IR.1943-4774.0000647
- [13] Brazilian Agricultural Research Corporation - EMBRAPA., Sistema Brasileiro de Classificação de Solos. 3<sup>a</sup> ed., Brasília, Embrapa, 2013, 353 P.
- [14] Willmott, C.J., On the validation of models. *Physical geography*, 2(2), pp. 184-194, 1981. DOI: 10.1080/02723646.1981.10642213
- [15] Varble, J.L. and Chávez, J.L., Performance evaluation and calibration of soil water content and potential sensors for agricultural soils in eastern Colorado. *Agricultural Water Management*, 101(1), pp. 93-106, 2011. DOI: 10.1016/j.agwat.2011.09.007
- [16] Richards, L.A., Diagnosis and improvement of saline and alkali soils. *Agriculture Handbook No. 60* [Online], Washington, United States Department of Agriculture (USDA), 1954. [date of reference: March 27<sup>th</sup> of 2018]. Available at: <https://www.ars.usda.gov/pacific-west-area/riverside-ca/us-salinity-laboratory/docs/handbook-no-60/>

**C.D.G.C. Almeida**, received the BSc. degree in Agronomy from the Federal Rural University of the Semi-Arid, Brazil, (1994), graduate degree in Agricultural Sciences at the Federal Rural University of Pernambuco, Brazil, (1998), MSc. in Agronomy (Soil Science) by Federal Rural University of Pernambuco, Brazil, (1998) and PhD in Irrigation and Drainage by Luiz de Queiroz College of Agriculture (ESALQ/USP), Brazil, with training in the modality-SWE PhD. at the University of Southern Queensland, Australia.

She is titular professor of Agricultural College Dom Agostinho Ikas (CODAI) of the Federal Rural University of Pernambuco (UFRPE). And she is permanent professor at Post Graduate program in Agricultural Engineering at UFRPE.

ORCID: 0000-0001-6073-3853

**D.M.O. Silva**, received the BSc. degree in Agricultural and Environmental Engineering from the Federal Rural University of Pernambuco, Brazil, (2012) and MSc. degree in Agricultural Engineering by Federal Rural University of Pernambuco, Brazil, (2017).

ORCID: 000-0001-5600-368X

**E.F.F. Silva**, received the BSc. degree in Agricultural Engineering from the Federal University of Lavras, Brazil, (1994), MSc. in Agricultural Engineering by Federal University of Paraíba, Brazil, (1997) and PhD in Irrigation and Drainage by Luiz de Queiroz College of Agriculture (ESALQ/USP), Brazil, (2002). He is professor of Department of Agricultural Engineering the Federal Rural University of Pernambuco (UFRPE) e permanent professor at Post Graduate program in Agricultural Engineering at UFRPE.

ORCID: 0000-0002-8652-503X

**J.A. Santos Júnior**, is BSc. at Agricultural Engineering at the Federal University of Campina Grande, Brazil, (2009), MSc. at Agricultural Engineering and PhD at Agricultural Engineering at the Federal University of Campina Grande, Brazil, (2013). He is professor of Agricultural Engineering Department of the Federal Rural University of Pernambuco, Brazil, (UFRPE). He is permanent professor at Post Graduate program in Agricultural Engineering at UFRPE.

ORCID: 0000-0002-1656-7103

**B.G. Almeida**, received the BSc. degree in Chemistry Science at the Federal Rural University of Pernambuco, Brazil, (1985) and BSc. degree in Industrial Chemistry at the Catholic University of Pernambuco, Brazil, (1990). MSc. at Agronomy (Soil Science) at the Federal Rural University of Pernambuco, Brazil, (1995) and PhD in Soil Science by Luiz de Queiroz College of Agriculture (ESALQ/USP), Brazil, with training in the modality-SWE PhD. at the University of Southern Queensland, Australia. He is professor of Agronomy Department of the Federal Rural University of Pernambuco (UFRPE). And he is permanent professor at Post Graduate program in Soil Science at UFRPE.

ORCID: 0000-0003-3260-0767

**R.N. Barbosa**, currently is a student of Agronomy at the Federal Rural University of Pernambuco, Brazil, (expected to complete in 2018). Participated in the Institutional Program of Scientific Initiation Grants from 2015 to 2017 with themes related to irrigation. Discipline's monitor irrigation and drainage of the agronomy graduation at the Federal Rural university of Pernambuco (2017 to present).

ORCID: 0000-0003-1746-7507



UNIVERSIDAD NACIONAL DE COLOMBIA

SEDE MEDELLÍN

FACULTAD DE MINAS

## Área Curricular de Medio Ambiente

### Oferta de Posgrados

Especialización en Aprovechamiento de  
Recursos Hidráulicos  
Especialización en Gestión Ambiental  
Maestría en Ingeniería Recursos Hidráulicos  
Maestría en Medio Ambiente y Desarrollo  
Doctorado en Ingeniería - Recursos Hidráulicos  
Doctorado Interinstitucional en Ciencias del Mar

Mayor información:

E-mail: [acma\\_med@unal.edu.co](mailto:acma_med@unal.edu.co)

Teléfono: (57-4) 425 5105